

# Lovibond® Water Analysis

Tintometer® Group



Lovibond® Comparator 2000+

## Simple Methods of Water Analysis

- ✓ Drinking Water
- ✓ Surface, Ground and Raw Water
- ✓ Sewerage and Domestic Effluents
- ✓ Waste Water and Effluents
- ✓ Boiler and Cooling Water
- ✓ Aquaculture



## System Components

Comparator instrument to bring the prepared sample and the glass filters together for colour matching



The Lovibond® Comparator 2000+ is a high quality instrument for visually matching the intensity of sample colour with Lovibond® glass filters; it includes an adjustable cell compartment for samples in cells of up to 40 mm path length. Lovibond® Nessleriser systems are longer path length instruments for matching a column of sample in a Nessler cylinder with Lovibond® glass filters; they are designed for measuring concentrations which are below the sensitivity of the Comparator 2000+.

Lovibond® comparator instruments include an integrated prism which causes the sample

and comparison fields to overlap, allowing enhanced colour discrimination and matching. The prism is ultrasonically sealed to prevent contamination of the optics. Both the Comparator 2000+ and the Nessleriser series include the facility to compensate for water samples which are turbid or tinted.



**Lighting unit (optional) to ensure constant viewing conditions for colour matching**

For consistent and accurate readings when using the Lovibond® Comparator System 2000+ it is important to use a constant light source for matching the sample with the glasses. Northern daylight (Southern daylight in the Southern hemisphere) is the optimum natural lighting for colour matching

although users should be aware that it will vary according to the time of day, the weather, the season and exact location. Only by using a Lovibond® lighting unit is it possible to guarantee uniform lighting conditions for colour matching, 24 hours a day and irrespective of ambient lighting. The Daylight Lighting Unit is a standardised bench-top light source which guarantees constant and uniform lighting conditions for colour matching. The Portable Lighting Unit is a constant light source powered by rechargeable batteries for colour matching in any location.



Lovibond Tintometer recommends the use of a standardised light source particularly when the sample is very pale in colour or with dark samples where relatively little light is transmitted through it or where the difference in colour between adjacent glasses is slight.

**Test disc containing a series of graded glass standards which have been pre-calibrated to give direct test readings**

The Lovibond® range includes a selection of over 200 water test discs covering different measuring ranges for more than 50 test parameters. The unique feature of Lovibond® test discs is that they incorporate coloured glass standards that are colour stable and not affected by UV light or extreme environmental conditions. Each individually graded glass standard represents a discrete step on the measurement range (as opposed to a continuous graduation), aiding colour discrimination and allowing greater accuracy of results.



The table on the following pages provides details of the commonly used Lovibond® test discs that are available for water analysis.

Individual test methods are supplied with the disc. For most tests, the discs are calibrated in mg/l (or parts per million) and the sample volume to be used is stated in the method. In certain tests, the calibration is in micrograms ( $\mu\text{g}$ ) so that the volume of the sample may be adjusted to cover the required concentration range.

**Sample container of the required path length**

Lovibond Tintometer supplies a range of precision fused glass and moulded optical cells and cylinders, in a range of dimensions and path lengths.

The table of Lovibond® water test discs include details of the container required for each test.



Order Code	Type	Product
35 42 43	DB424/S	Square 13.5 mm, 10 ml moulded glass cells with stoppers (pack of 5)
35 20 40		Square 13.5 mm, 10ml moulded plastic cells with stoppers (pack of 5)
60 68 90	W680/OG/40	Fused cell, 40 mm path length calibrated at 20 ml
60 67 80	W680/OG/2.5	Fused cell, 2.5 mm path length
60 67 90	W680/OG/5	Fused cell, 5 mm path length
60 68 60	W680/OG/25	Fused cell, 25 mm path length
35 30 80	AF 306/P	Pair of cylinders (50 ml, 113mm) with glass anti-meniscus plungers for Nessleriser 2150
35 42 00	DB 420	Pair of cylinders (250 ml) with glass anti-meniscus plungers for Nessleriser 2250
35 42 30	DB 423	Pair of cylinders 100 ml (288 mm) (ASTM D 1209) with glass anti-meniscus plungers for Nessleriser 1209

**Reagents, specific to the test, which produce a colour change in the sample**

Included in the Lovibond® Comparator System 2000 is a comprehensive range of chemical reagents which develop the colour in the water sample. For many tests, reagents are available in a convenient tablet form, each tablet containing the correct mix of reagent, buffers and catalysts to ensure accurate dosing. The majority of Lovibond® tablet reagents are available in blister packs for a long shelf-life.


**Accessories, as required**

There are a range of accessories for use with the Lovibond® Comparator System 2000.

Order Code	Type	Product
17 02 60	DB 426	Cell stand for 10 ml moulded cells, to hold 10 cells
17 02 90	AF 306/S	Stand for 12 Nessler cylinders
36 41 10		Glass stirring rod 4"/10 cm for comparator cells
36 40 80		Glass stirring rod 8"/20 cm for Nessler cylinders
36 41 00		Plastic stirring rod 5"/13 cm
38 02 30		Cleaning brush 4"/10 cm
38 00 30		Cleaning brush 8"/20 cm

## Lovibond® Comparator System 2000+

Colorimetric testing is a widely used method of quantitative water analysis which depends on measuring the intensity of colour, produced by the action of an appropriate chemical reagent, to determine the concentration of a particular chemical present in a sample.

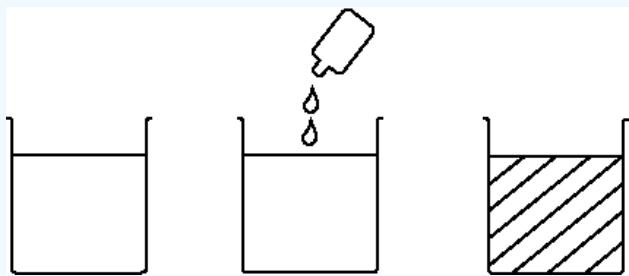

A known volume  
of sample

Add appropriate  
reagent

Measure intensity  
of colour produced


Lovibond Tintometer offers a selection of equipment which can be used to measure the depth of colour in a treated sample to give a quantitative answer:

### Lovibond® Comparator System 2000+


Based on visual comparison with coloured glass filters, which are calibrated to allow direct measurement of concentration levels.

### Using the System

1 Follow the test method for sample preparation, adding the specified reagent to a known volume of sample in the appropriate sample container.




2 Insert the Lovibond® test disc into the comparator instrument.



3 Place the sample container in the right hand comparator compartment, and, if specified in the test method, a cell containing a blank of water or untreated sample in the left hand side.



4 Using standardised lighting, rotate the disc until the closest colour match with the sample is obtained.



5 The value will be shown in the window in the comparator instrument.




## Colorimetric Chemical Analysis using Precalibrated Coloured Glass Filters



- ✓ The equipment is easily used and quick to obtain results.
- ✓ It gives dependable measurements with guaranteed repeatability.
- ✓ It is compact, robust and easily portable.
- ✓ Reagents are mostly available in a convenient tablet form allowing accurate dosage.
- ✓ Set up costs are low and it is inexpensive to operate.
- ✓ Additional measurement ranges and tests are readily added, for more than 50 different parameters.
- ✓ The glass filters used for colour matching are colour stable and not affected by UV light.
- ✓ The comparator system can be used with turbid samples, unlike photometric systems.
- ✓ It includes optional lighting units to guarantee constant viewing conditions for colour matching.
- ✓ The test discs can be certified periodically under an ISO 9001:2000 QA procedure.

For more than 60 years the Lovibond® Comparator System has been used around the world for chemical analysis of water. Today it remains a popular choice for water analysis in all environments, offering a simple and flexible approach which gives reliable results in both laboratory and field testing:

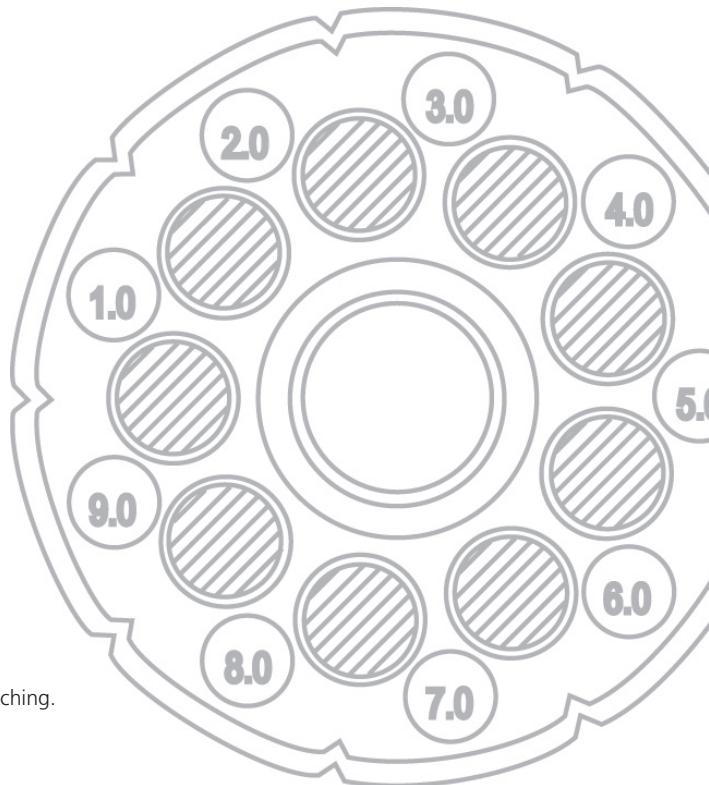

## Nessleriser Systems

The Lovibond® Nessleriser Systems are based on the Comparator 2000+. They have a longer path length and are capable of measuring concentrations below the sensitivity of the standard Comparator.

Like the Comparator 2000+ the Nessleriser Systems include a prism to allow colour matching in a single field of view. Systems use either natural light or an electronic daylight unit for a consistant light source.

2150 systems use cells with a path length of 113mm and are compatible with any Comparator 2000+ disc with the prefix "N".

2250 systems use cells with a path length of 250mm and are compatible with any Comparator 2000+ disc with the prefix "C".

The AF327 system is specifically designed for Hazen (Platinum-Cobalt) testing to the ASTM D1209 standard and uses a path length of 288mm.



Order Code	Product	Path Length
172150	Nessleriser 2150 System	113mm
172030	Nessleriser 2150 Daylight System	113mm
172250	Nessleriser 2250 System	250mm
172040	Nessleriser 2250 Daylight System	250mm
433270	Nessleriser AF327	288mm
<b>Accessories</b>		
353060	AF306 Nessler Tubes	113mm
353080	AF306/P Nessler Tubes with Plungers	113mm
354200	DB420 Nessler Tubes with Plungers	250mm
354230	DB423 Nessler Tubes with Plungers	288mm

## Lovibond® Comparator 2000+ Kits

A wide range of single and multi parameter test kits based on the Comparator 2000 are available. Kits are supplied in a robust carry case with all necessary cells, reagents, discs, instructions and accessories (including additional Nesslerisers and MiniKit titration kits where necessary).

Part numbers for all available single parameter kits can be found in the Table of Water Test Discs and Kits on pages 6 to 14. Listed below are examples of kits for applications across the water industry. Bespoke kits containing customer specified tests can also be supplied on request. Please contact the local Lovibond® representative for further details.

## Lovibond® 2000+ Leisure Water Kits

Order Code	Description	Tests	Range
411160	AF116B Chlorine / pH Kit	Chlorine pH	0-4 mg/l 6.8-8.4
416570	AF113C Bromine / pH Kit	Bromine pH	0-6 mg/l 6.8-8.4
411290	AF129 Balanced Water Kit	Chlorine pH Alkalinity Calcium Hardness	0-4 mg/l 6.8-8.4 10-500 mg/l 10-500 mg/l



## Lovibond® 2000+ Environmental / Industrial Water Kits

Order Code	Description	Tests	Range
411120	AF112A Chlorine Free and Combined Kit	Chlorine	0-1 mg/l
416241	AF112G Shipboard Chlorine Kit	Chlorine	0.02-0.5 mg/l
413570	AF357 Potable Water Kit	Chloride Chlorine Hardness Hazen pH	0-5000 mg/l 0.02-4 mg/l 0-500 mg/l 10-90 mg/l 6-8.4
413580	AF358 Sewage and Domestic Effluent Kit	Ammonia Chlorine Nitrite Permanganate pH Sulphide	0-1 mg/l 0.1-10 mg/l 0.05-0.5 mg/l 0-60 mg/l BOD 4-9.6 0-0.5 mg/l
411090	AF110 High and Low Chlorine Kit	Chlorine Chlorine (total)	0-1 mg/l 5-50 mg/l
411000	AF100 Water Disinfection Kit	Chlorine pH Sodium Hypochlorite	0.2-50 mg/l 6.8-8.4 2-16%



**Table of Lovibond® Water Test Discs**

ORDER CODE	TEST (Instrument)	DISC CODE	DISC READINGS / RANGE COVERED	REAGENT CODE	CHEMICAL METHOD BASED ON	ACCESSORIES REQUIRED	APPLICATIONS	KIT PART NUMBER
23 02 05	<b>ALUMINIUM</b> (Comparator)	3/127A 3/115 3/108	0, 0.05, 0.10, 0.15, 0.20, 0.25, 0.30, 0.40, 0.50 mg/l 0.1, 0.2, 0.3, 0.4, 0.5, 0.6, 0.7, 0.8 mg/l & "blank" 0, 0.05, 0.1, 0.15, 0.2, 0.25, 0.3, 0.4 mg/l	517601BT	Aluminium Tablets Haematoxylin Catechol Violet	13.5 mm cells DB 424 13.5 mm cells DB 424 13.5 mm cells DB 424	Water treatment processes	411570
23 15 00								
23 10 80								
28 38 90	<b>ALUMINIUM</b> (Nessleriser 2150)	NX	0.5, 1, 1.5, 2, 2.5, 3, 3.5, 4, 4.5 µg		Haematoxylin	Nessler cylinders AF 306/P		
23 58 00	<b>AMINES</b> (Comparator)	3/58 3/64	1, 2, 3, 4, 5, 6, 7, 8, 10 mg/l as octadecylamine 0, 0.25, 0.5, 1, 2 mg/l as octadecylamine	511010 56R013290	Amine Tablets Methyl Orange	Extraction tube AF 260 13.5 mm cells DB 424	Boiler water & feed water	412740
23 64 00								56K013201
23 00 60	<b>AMMONIA</b> (Comparator)	3/112 3/113 3/125 3/166	0, 0.05, 0.10, 0.15, 0.20, 0.25, 0.30, 0.35, 0.40 mg/l NH <sub>4</sub> 0, 0.1, 0.2, 0.3, 0.4, 0.5, 0.6, 0.8, 1.0 mg/l N 0, 1, 2, 3, 4, 5, 6, 8, 10 mg/l N 2, 4, 6, 8, 10, 12, 14, 16, 20 mg/l N	517611BT " " "	Ammonia Tablets Ammonia Tablets Ammonia Tablets Nessler's Reagent	40 mm cells DB 428 13.5 mm cells DB 424 2.5 mm cells W680/OG/2.5 13.5 mm cells DB 424	Fish farms/aquaria Industrial effluent, sewage leaks Industrial effluent, sewage leaks	411580 411590 411600
23 00 70								
23 01 80								
23 06 60								
28 31 10	<b>AMMONIA</b> (Nessleriser 2150)	NAA NAB NAC NAD	1, 2, 3, 4, 5, 6, 7, 8, 10 µg NH <sub>3</sub> 10, 12, 14, 16, 18, 20, 22, 24, 26 µg NH <sub>3</sub> 28, 32, 36, 40, 44, 48, 52, 56, 60 µg NH <sub>3</sub> 60, 65, 70, 75, 80, 85, 90, 95, 100 µg NH <sub>3</sub>	465200, 466101 " " " " " " "	Nessler's Reagent Nessler's Reagent Nessler's Reagent Nessler's Reagent	Nessler cylinders AF 306/P Nessler cylinders AF 306/P Nessler cylinders AF 306/P Nessler cylinders AF 306/P	Water courses as an indicator of organic pollution " " " " " "	411580 411590 411600
28 31 20								
28 31 30								
28 31 40								
23 06 30	<b>BAQUACIL*</b> (Comparator)	3/163	0, 20, 25, 30, 35, 40, 45, 50, 75 ppm	515890	Baquatest Tablets	13.5 mm cells DB 424	Swimming Pools	
23 02 20	<b>BORON</b> (Comparator)	3/129	0, 0.2, 0.4, 0.6, 0.8, 1.0, 1.5, 2.0, 2.5 mg/l	515790, 515800	Boron Tablets	13.5 mm cells DB 424	Drinking water and hydroponics	
23 53 10	<b>BROMINE</b> (Comparator)	3/53A 3/53B 3/53C	0.2, 0.4, 0.6, 0.8, 1.0, 1.2, 1.4, 1.6, 2.0 mg/l 1, 2, 3, 4, 5, 6, 7, 8, 10 mg/l 0.5, 1.0, 1.5, 2.0, 2.5, 3.0, 4.0, 5.0, 6.0 mg/l	511050BT " "	DPD Tablets DPD Tablets DPD Tablets	13.5 mm cells DB 424 13.5 mm cells DB 424 13.5 mm cells DB 424	Swimming Pools and spas Swimming Pools and spas	416530 416540 411080
23 53 20								
23 53 30								
23 89 00	<b>CADMIUM</b> (Comparator)	3/89 ‡	0.5, 1, 1.5, 2, 2.5, 3, 4, 5 µg		Dithizone/Potassium Cyanide	13.5 mm cells DB 424	Effluents	
23 10 20	<b>CHEMICAL OXYGEN DEMAND</b> (Comparator)	4/21‡ 4/21A ‡ 4/21B ‡ 4/21C ‡	200, 300, 400, 500, 600 ppm 100, 125, 150, 175, 200, 225, 250, 275, 300 ppm 40, 50, 60, 70, 80, 90, 100, 110, 120 ppm 10, 20, 30, 40 ppm		Dichromate oxidation Dichromate oxidation Dichromate oxidation Dichromate oxidation	13.5 mm cells DB 424 13.5 mm cells DB 424 13.5 mm cells DB 424 13.5 mm cells DB 424	Dairy and malting effluents Dairy and malting effluents Dairy and malting effluents Dairy and malting effluents	
23 10 40								
23 10 50								
23 71 00	<b>CHLORIDE</b> (Comparator)	3/71 3/72	10, 25, 50, 75, 100, 150, 200 mg/l 2.5, 5, 7.5, 10, 15, 20, 40, 60, 80 mg/l	464801 464801	Mercuric Thiocyanate Mercuric Thiocyanate	13.5 mm cells DB 424 40 mm cells DB 428	Salinity of water Salinity of water	
23 72 00								
28 37 90	<b>CHLORIDE</b> (Nessleriser 2150)	NOV	1, 2, 3, 4, 5, 6, 7, 8, 10 mg/l	464801	Mercuric Thiocyanate	Nessler cylinders AF 306/P	Salinity of water	

\* Baquacil is a trade mark of Zeneca Biocides

† Laboratory method; not suitable as a test kit

**Table of Lovibond® Water Test Discs**

ORDER CODE	TEST (Instrument)	DISC CODE	DISC READINGS / RANGE COVERED	REAGENT CODE	CHEMICAL METHOD BASED ON	ACCESSORIES REQUIRED	APPLICATIONS	KIT CODE
23 40 10	CHLORINE (Comparator) DPD	3/40A	0.1, 0.2, 0.3, 0.4, 0.5, 0.6, 0.7, 0.8, 1.0 mg/l *	511050BT, 511080BT	DPD Tablets	"	Drinking water	411120
23 41 40		3/40J	0.1, 0.2, 0.3, 0.4, 0.6, 0.8, 1.0, 1.5, 2.0 mg/l *	"	DPD Tablets	"		411125
23 40 90		3/40S	1.0, 1.2, 1.4, 1.6, 1.8, 2.0, 2.5, 3.0, 4.0 mg/l *	"	DPD Tablets	"		411124
23 40 20		3/40B	0.2, 0.4, 0.6, 1.0, 1.5, 2.0, 2.5, 3.0, 4.0 mg/l *	"	DPD Tablets	"		411124
23 40 60		3/40E	0.02, 0.04, 0.06, 0.08, 0.1, 0.15, 0.2, 0.25, 0.3 mg/l *	"	DPD Tablets	"		411125
29 59 20		-	0.02, 0.04, 0.06, 0.08, 0.1, 0.2, 0.3, 0.4, 0.5 mg/l *	"	DPD Tablets	"		
23 40 70		3/40F	0.2, 0.25, 0.3, 0.35, 0.4, 0.5, 0.6, 0.7, 0.8 mg/l *	"	DPD Tablets	"		
23 40 81		3/40IN	2, 3, 4, 5, 6, 7, 8, 9, 10 mg/l *	"	DPD Tablets	"		
23 39 30		3/40K	0.5, 1.0, 1.5, 2.0, 2.5, 3.0, 4.0, 5.0, 6.0 mg/l *	"	DPD Tablets	"		411121
23 39 20		3/40P	2.0, 2.3, 2.5, 2.7, 3.0, 3.2, 3.6, 4.0, 5.0 mg/l *	"	DPD Tablets	"		411127
23 20 60		3/2APH	2, 3, 4, 5, 6, 7, 8, 9, 10 mg/l total Cl <sub>2</sub>	5117721BT	Potassium Iodide Tablets	"		418883
23 20 70		3/2ARP	5, 10, 15, 20, 25, 30, 35, 40, 50 mg/l total Cl <sub>2</sub>	"	Potassium Iodide Tablets	"		418881
23 20 90		3/2ID	5, 10, 25, 50, 75, 100, 150, 200, 250 mg/l total Cl <sub>2</sub>	"	Potassium Iodide Tablets	"		418880
23 21 10		3/2Hypo	2, 4, 6, 8, 10, 12, 14, 16% w/w available Cl <sub>2</sub>	"	Potassium Iodide Tablets	"		411390
23 25 10		3/25A	0.1, 0.2, 0.3, 0.4, 0.5, 0.6, 0.7, 0.8, 1.0 mg/l		Neutral o-Tolidine**			
23 25 20		3/25B	0.25, 0.5, 1.0, 1.5, 2.0, 2.5, 3.0, 4.0, 5.0 mg/l		Neutral o-Tolidine**			
23 20 10		3/2A	0.1, 0.2, 0.3, 0.4, 0.5, 0.6, 0.7, 0.8, 1.0 mg/l		Acid o-Tolidine**			
23 20 80		3/2B	1.2, 1.4, 1.6, 1.8, 2.0 mg/l		Acid o-Tolidine**			
23 20 20		3/2AB	0.15, 0.25, 0.5, 0.75, 1.0, 1.25, 1.5, 1.75, 2.0 mg/l		Acid o-Tolidine**			
23 20 50		3/2APC	1.0, 1.5, 2.0, 2.5, 3.0, 3.5, 4.0, 4.5, 5.0 mg/l		Acid o-Tolidine**			
23 20 30		3/2APA	0.02, 0.04, 0.06, 0.08, 0.1, 0.15, 0.2, 0.25, 0.3 mg/l		Acid o-Tolidine**			
23 20 40		3/2APB	0.2, 0.25, 0.3, 0.35, 0.4, 0.5, 0.6, 0.7, 0.8 mg/l		Acid o-Tolidine**			
28 34 50	CHLORINE DPD (Nessleriser 2150)	NDPB	0.01, 0.02, 0.03, 0.04, 0.05, 0.06, 0.07, 0.08, 0.1 mg/l	511230BT, 511250BT	DPD Tablets	"	Portable water treatment	
28 34 60		NDPC	0.02, 0.04, 0.06, 0.08, 0.1, 0.12, 0.14, 0.16, 0.2 mg/l	"	DPD Tablets	"	Portable water treatment	
28 34 40		NDP	0.05, 0.1, 0.15, 0.2, 0.25, 0.3, 0.35, 0.4, 0.5 mg/l	"	DPD Tablets	"	Portable water treatment	
28 34 70		NDPD	0.1, 0.2, 0.3, 0.4, 0.5, 0.6, 0.7, 0.8, 1.0 mg/l	"	DPD Tablets	"	Portable water treatment	
28 33 10		NCA	0.01, 0.02, 0.03, 0.04, 0.05, 0.06, 0.07, 0.08, 0.09 mg/l		Acid o-Tolidine**			
28 33 30		NCB	0.1, 0.15, 0.2, 0.25, 0.3, 0.35, 0.4, 0.45, 0.5 mg/l		Acid o-Tolidine**			
28 33 20		NCAB	0.02, 0.04, 0.06, 0.08, 0.1, 0.2, 0.3, 0.4, 0.5 mg/l		Acid o-Tolidine**			
28 34 90	CHLORINE (Nessleriser 2250)	CBA	0.002, 0.004, 0.006, 0.008, 0.01, 0.015, 0.02, 0.025, 0.03 mg/l	471056	DPD Liquid	"	Aquaria, effluents	250 mm cylinders DB 420

\* Can be used for free, combined and total chlorine measurements

\*\* The use of o-Tolidine is controlled in the UK by the Carcinogenic Substances Regulations 1967

**Table of Lovibond® Water Test Discs**

ORDER CODE	TEST (Instrument)	DISC CODE	DISC READINGS / RANGE COVERED	REAGENT CODE	CHEMICAL METHOD BASED ON	ACCESSORIES REQUIRED	APPLICATIONS	KIT PART NUMBER
29 22 60	CHLORINE DIOXIDE (Comparator)	3/40AD	0.19, 0.38, 0.57, 0.76, 0.95, 1.14, 1.33, 1.52, 1.9 mg/l	511050BT, 512170BT	DPD Tablets	13.5 mm cells DB 424	Water treatment, cooling towers	56K014501
29 21 60		3/40BD	0.38, 0.76, 1.14, 1.9, 2.85, 3.8, 4.75, 5.7, 7.6 mg/l	" "	DPD Tablets	13.5 mm cells DB 424	Water treatment, cooling towers	
29 79 70		3/40ED	0.04, 0.08, 0.11, 0.15, 0.19, 0.28, 0.38, 0.48, 0.57 mg/l	" "	DPD Tablets	40 mm cells DB 428	Water treatment, cooling towers	419811
23 05 70		3/157	0.25, 0.5, 0.75, 1.0, 1.25, 1.5, 2.0, 3, 5.0 mg/l	5117721BT, 512170BT	Potassium Iodide Tablets	40 mm cells DB 428	Water treatment, cooling towers	421540
28 34 50	CHLORINE DIOXIDE (Nessleriser 2150)	NDPB	0.01, 0.02, 0.03, 0.04, 0.05, 0.06, 0.07, 0.08, 0.1 mg/l as Cl <sub>2</sub>	5111230BT, 512170BT	DPD Tablets	Nessler cylinders AF 306/P		
28 34 60		NDPC	0.02, 0.04, 0.06, 0.08, 0.1, 0.12, 0.14, 0.16, 0.2 mg/l as Cl <sub>2</sub>	" "	DPD Tablets	Nessler cylinders AF 306/P		
28 34 40		NDP	0.05, 0.1, 0.15, 0.2, 0.25, 0.3, 0.35, 0.4, 0.5 mg/l as Cl <sub>2</sub>	" "	DPD Tablets	Nessler cylinders AF 306/P		
23 59 00	CHROMIUM (Comparator)	3/79	10, 20, 30, 40, 50, 60, 70, 80, 100 µg		Diphenylcarbazide	13.5 mm cells DB 424	Plating effluents, Chromium VI and total chromium	413630
23 10 60		4/35	100, 150, 200, 250, 300, 350, 400, 500, 600 mg/l Cr as sodium chromate		Colour of chromate ion	13.5 mm cells DB 424	Heating systems where chromates used as a rust inhibitor	
28 31 70	CHROMIUM (Nessleriser 2150)	NOK	2, 3, 4, 5, 6, 7, 8, 9, 10 µg		Diphenylcarbazide	Nessler cylinders AF 306/P		
23 31 00	COBALT (Comparator)	3/31 †	10, 25, 50, 75, 100, 125, 150, 175, 200 µg		Thiocyanate	13.5 mm cells DB 424		
28 38 60	COBALT (Nessleriser 2150)	NTA ‡	1, 2, 3, 4, 5, 6, 7, 8, 9 µg		Nitroso-R salt	Nessler cylinders AF 306/P		
28 38 70		NTB ‡	10, 12.5, 15, 17.5, 20, 22.5, 25, 27.5, 30 µg		Nitroso-R salt	Nessler cylinders AF 306/P		
23 00 50	COPPER (Comparator)	3/106	0, 0.1, 0.2, 0.3, 0.4, 0.5, 0.6, 0.8, 1.0 mg/l	51260BT	Copper/Zinc Low Range Tablets	13.5 mm cells DB 424	Industrial water/waste water	411620
23 00 40		3/110	0, 0.5, 1.0, 1.5, 2.0, 2.5, 3.0, 3.5, 4.0 mg/l	512240BT	Copper/Zinc High Range Tablets	13.5 mm cells DB 424	Industrial water/waste water	56K014801
23 06 80		3/168	0.1, 0.2, 0.3, 0.4, 0.5, 0.6, 0.7, 0.8, 1.0 mg/l	517692BT	Copper Tablets	40 mm cells DB 428		
23 04 50		3/149	0.5, 1.0, 1.5, 2.0, 2.5, 3.0, 3.5, 4.0, 5.0 mg/l	517692BT	Copper Tablets	13.5 mm cells DB 424		
23 39 00		3/39	2.5, 5, 10, 15, 20, 25, 30, 40, 50 µg		Zinc Dibenzylidithio-carbamate	13.5 mm cells DB 424	Trade effluents	
23 05 00		3/5	2.5, 5, 10, 15, 20, 25, 30, 40, 50 µg		Sodium Diethylidithio-carbamate	13.5 mm cells DB 424		
23 10 90		3/109	0.0125, 0.025, 0.05, 0.075, 0.1, 0.125, 0.15, 0.2, 0.25 mg/l		Copper 3/109 Tablets	Special extractor AF 262	Domestic water supplies	
28 34 10	COPPER (Nessleriser 2150)	NDA	2.5, 5.0, 10, 15, 20, 25, 30, 35, 40 µg		Dithio-oxamide	Nessler cylinders AF 306/P		
28 34 30		NDB	30, 35, 40, 50, 60, 70, 80, 90, 100 µg		Dithio-oxamide	Nessler cylinders AF 306/P		
23 33 00	CYANIDE (Comparator)	3/33 †	0.05, 0.1, 0.2, 0.3, 0.4, 0.5, 0.6, 0.8, 1.0 mg/l		Benzidine Pyridine	13.5 mm cells DB 424	Not for use in UK	
23 86 00		3/86	0.05, 0.1, 0.2, 0.3, 0.4, 0.5, 0.6, 0.8, 1.0 mg/l		p-Phenylenediamine dihydrochloride	13.5 mm cells DB 424	Effluents. Measures free and simple complexes	413620
28 36 60	CYANIDE (Nessleriser 2150)	NOC ‡	0.02, 0.04, 0.06, 0.08, 0.1, 0.12, 0.14, 0.16, 0.2 mg/l	513220BT, 461181	Pyridine pyrazolone	Nessler cylinders AF 306/P	River water, sewage and trade effluents	
23 04 60	DEHA (Comparator)	3/150	8, 16, 24, 32, 40, 48, 56, 64, 80 µg/l. Disc reading should be multiplied by 2 for true DEHA concentration		Iron reduction	40 mm cells DB 428	Oxygen scavenger - boiler water	416400
23 48 00	DETERGENTS (Comparator)	3/48 †	1, 2, 3, 4, 6, 8, 10, 12 16 mg/l active material		Methylene Blue	13.5 mm cells DB 424	Measures anionic detergents	

† Laboratory method; not suitable as a test kit

Table of Lovibond® Water Test Discs

ORDER CODE	TEST (Instrument)	DISC CODE	DISC READINGS / RANGE COVERED	REAGENT CODE	CHEMICAL METHOD BASED ON	ACCESSORIES REQUIRED	APPLICATIONS	KIT PART NUMBER
29 68 10	DICHLOROPHEN (PANACIDE*) IN WATER (Comparator)	3/57B	20, 30, 40, 50, 60, 70, 80, 90, 100 mg/l		4-amino antipyrine	5 mm cells W680/OG/5	Cooling towers, air conditioning plant etc	
28 37 40	FLUORIDE (Nessleriser 2150)	NOO	0.5, 0.6, 0.7, 0.8, 0.9, 1.0, 1.1, 1.2, 1.3 mg/l 0.0, 0.2, 0.4, 0.6, 0.8, 1.0, 1.2, 1.4, 1.6 mg/l	511400, 511410 " " "	Acid alizarin zirconium Tablets	Nessler cylinders AF 306/P	Cooke, Dixon and Sawyer method	
28 37 80		NOM	0.2, 0.3, 0.4, 0.5, 1.1, 1.2, 1.3, 1.4, 1.5 mg/l	" "	Acid alizarin zirconium Tablets	Nessler cylinders AF 306/P	Tablet method for natural and added fluoride	416070
23 10 70	HARDNESS, TOTAL (Comparator)	NOT		" "	Acid alizarin zirconium Tablets	Nessler cylinders AF 306/P	Control of drinking water fluoridation	
24 28 00	HAZEN SCALE (Comparator)	4/28	0, 5, 10, 15, 20, 25, 30, 40, 60 mg/l CaCO <sub>3</sub>		Hardness Eriochrome Powder	13.5 mm cells DB 424	Hardness in boiler water	
28 41 70	HAZEN SCALE (Nessleriser 2150)	NSH	10, 20, 30, 40, 50, 60, 70, 80, 90 mg Pt/l	N/A	Straight colour match to sample	40 mm cells DB 428*	APHA, ASTM & British Standards	
28 41 20		NSB	70, 85, 100, 125, 150, 175, 200, 225, 250 mg Pt/l	" "	Straight colour match to sample	Nessler cylinders AF 306/P**	APHA, ASTM & ISO Standards	433250
28 41 30		NSX	50, 60, 70, 80, 100, 150, 200, 250, 300 mg Pt/l	" "	Straight colour match to sample	Nessler cylinders AF 306/P**	APHA, ASTM & ISO Standards	"
28 41 50	HAZEN SCALE (Nessleriser 2250)	CAA	0, 2.5, 5, 7.5, 10, 15, 20, 25, 30 mg Pt/l	N/A	Straight colour match to sample	Nessler cylinders AF 306/P**	APHA, ASTM & ISO Standards	433280
28 41 60		CAB	30, 35, 40, 45, 50, 55, 60, 65, 70 mg Pt/l	" "	Straight colour match to sample	250 mm cylinders DB 420**	APHA, ASTM & ISO Standards	"
28 39 70	HAZEN SCALE (Nessleriser 1209)	1209/1	0, 2.5, 5, 7.5, 10, 15, 20, 25, 30 mg Pt/l	N/A	Straight colour match to sample	250 mm cylinders DB 420**	APHA, ASTM & ISO Standards	433270
28 39 80		1209/2	30, 35, 40, 45, 50, 55, 60, 65, 70 mg Pt/l	" "	Straight colour match to sample	100 ml cylinders DB 423 **	Conforms to path length requirements specified in ASTM D 1209	
23 01 90	HYDRAZINE (Comparator)	3/126	0, 0.05, 0.1, 0.15, 0.2, 0.25, 0.3, 0.4, 0.5 mg/l	462910	Hydrazine test powder	13.5 mm cells DB 424	Boiler water	56K015001
23 02 90		3/135	0.02, 0.04, 0.06, 0.08, 0.1, 0.12, 0.14, 0.16, 0.2 mg/l	" "	Hydrazine test powder	40 mm cells DB 428	Boiler water	
23 85 00		3/85	0, 0.1, 0.2, 0.3, 0.4, 0.5, 0.6, 0.8, 1.0 mg/l	461261	p-dimethyl-amino-benzaldehyde	13.5 mm cells DB 424	Simple single reagent	
28 37 00	HYDRAZINE (Nessleriser 2150)	NOH	0, 0.5, 1, 2, 3, 4, 6, 8, 10 µg	" "	p-dimethyl-amino-benzaldehyde	Nessler cylinders AF 306/P	Boiler water	
23 50 00	HYDROGEN PEROXIDE (Comparator)	3/50A	0.05, 0.1, 0.15, 0.2, 0.25, 0.3, 0.35, 0.4, 0.5 mg/l	512380	Hydrogen Peroxide Low Range Tablets	13.5 mm cells DB 424		56K015201
23 50 10		3/50B	0.1, 0.2, 0.3, 0.4, 0.6, 1.0, 1.5, 2.0, 3.0 mg/l	" "		13.5 mm cells DB 424		411350
23 50 20		3/50E	0.01, 0.02, 0.03, 0.04, 0.05, 0.07, 0.09, 0.12, 0.15 mg/l	" "		40 mm cells DB 428		
23 00 80		3/114	2, 4, 6, 8, 10, 12, 14, 16, 20 mg/l	513530, 513010	Hydrogen Peroxide High Range Tablets	13.5 mm cells DB 424		411481
23 00 90		3/115	10, 20, 30, 40, 50, 60, 70, 80, 100 mg/l	513530, 513010	" "	13.5 mm cells DB 424		
29 64 70		3/105	3, 5, 10, 15, 20, 30, 40, 50, 70 mg/l	Potassium Titanium Oxalate	" "	13.5 mm cells DB 424	Sewage treatment	411480
23 77 10	IODINE (Comparator)	3/77A	0.4, 0.7, 1.1, 1.4, 1.8, 2.2, 2.5, 2.9, 3.6 mg/l	511050BT	DPD Tablets	13.5 mm cells DB 424		
23 77 20		3/77B	0.7, 1.4, 2.2, 3.6, 5.4, 7.2, 9.0, 11, 14 mg/l	DPD Tablets	13.5 mm cells DB 424			

\* Registered Trade Mark of Coalite Chemicals

\*\* Use of a standardised lighting unit is recommended for pale coloured samples

**Table of Lovibond® Water Test Discs**

ORDER CODE	TEST (Instrument)	DISC CODE	DISC READINGS / RANGE COVERED	REAGENT CODE	CHEMICAL METHOD BASED ON	ACCESSORIES REQUIRED	APPLICATIONS	KIT PART NUMBER
22 03 80	IRON (Comparator)	3/144	0.02, 0.04, 0.06, 0.08, 0.1, 0.15, 0.2, 0.25, 0.3 mg/l	515370BT	Iron Low Range Tablets	40 mm cells DB 428	Measures total soluble iron	413780
23 01 00		3/116	0.1, 0.2, 0.3, 0.4, 0.5, 0.6, 0.7, 0.8, 1.0 mg/l	515370BT, 515420	Iron Low Range Tablets	13.5 mm cells DB 424	Measures total soluble iron	413790
23 01 10		3/117	1, 2, 3, 4, 5, 6, 7, 8, 10 mg/l	515380	Iron High Range Tablets	13.5 mm cells DB 424	Measures total soluble iron	
23 88 00		3/88	0.05, 0.1, 0.15, 0.2, 0.25, 0.3, 0.5, 0.75, 1.0 mg/l		o-Phenanthroline	40 mm cells DB 428	Measures ferrous and ferric iron	
23 06 00		3/6	10, 20, 30, 40, 50, 60, 70, 80, 100 µg		Thioglycollic acid	13.5 mm cells DB 424	Measures total iron	
23 10 10		APFE	0.5, 1, 1.5, 2, 2.5, 3, 3.5, 4.5, 5 mg/l		Thioglycollic acid	40 mm cells DB 428	Measures total iron	
23 11 00		3/11	2, 4, 6, 8, 10, 12.5, 15, 20, 25 µg		Thiocyanate	13.5 mm cells DB 424	Measures ferric iron	
23 05 90		3/159	10, 20, 30, 40, 50, 60, 80, 110, 140 µg		o-Phenanthroline	13.5 mm cells DB 424	Measures ferric iron	
28 37 20	IRON (Nessleriser 2150)	NOL	0.01, 0.02, 0.03, 0.04, 0.05, 0.06, 0.07, 0.08, 0.10 mg/l	515370BT, 515420	Iron Low Range Tablets	Nessler cylinders AF 306/P	Measures total soluble iron	
28 35 10		NEA	2, 4, 6, 8, 10, 12, 14, 16, 18 µg		Thioglycolic Acid	Nessler cylinders AF 306/P	Measures total iron	
28 35 30		NEB	20, 25, 30, 35, 40, 45, 50, 55, 60 µg		Thioglycolic Acid	Nessler cylinders AF 306/P	Measures total iron	
28 35 20		NEAB	5, 10, 15, 20, 25, 30, 40, 50, 60 µg		Thioglycolic Acid	Nessler cylinders AF 306/P	Measures total iron	
23 05 30	LEAD (Comparator)	3/153 ‡	1, 2, 4, 6, 8, 10, 12, 16, 20 µg		Dithizone/Cyanide	13.5 mm cells DB 424	Low levels in drinking water	
23 28 00	MAGNESIUM (Comparator)	3/28	0, 1, 2, 3, 4, 5, 7, 10 mg/l		Titan Yellow	13.5 mm cells DB 424		
23 06 90	MANGANESE (Comparator)	3/169	0, 0.5, 1.0, 1.5, 2.0, 2.5, 3.0, 3.5, 4.0 mg/l	517621BT	Manganese LR Tablets	13.5 mm cells DB 424	Total manganese in natural and industrial water supplies	56K015601
23 21 50		3/21	5, 10, 15, 20, 25, 30, 40, 50, 60 µg		Formaldoxime Hydrochloride	13.5 mm cells DB 424		
23 55 00		3/55	0.03, 0.05, 0.09, 0.12, 0.15, 0.18, 0.21, 0.25, 0.3 µg		Luecomalachite green	13.5 mm cells DB 424		
28 39 20	MANGANESE (Nessleriser 2150)	NZZ	0.025, 0.05, 0.075, 0.1, 0.15, 0.2, 0.3, 0.4, 0.5 mg/l		Formaldoxime Hydrochloride	Nessler cylinders AF 306/P		
28 39 40	MANGANESE (Nessleriser 2250)	CCA	0.05, 0.1, 0.15, 0.2, 0.25, 0.3, 0.5, 0.75, 1.0 mg/l		Formaldoxime	250 mm cylinders DB 420		
23 06 20	MOLYBDATE (Comparator)	3/162	0, 1, 2, 3, 4, 5, 6, 8, 10 mg/l MoO <sub>4</sub>	56R015750	Dihydroxybenzene disulphonic acid	40 mm cells DB 428	Industrial water systems	56K015701
23 03 20		3/137	5, 10, 15, 20, 25, 30, 35, 40, 50 mg/l MoO <sub>4</sub>	517631BT	Molybdate Tablets	40 mm cells DB 428	Industrial water systems	56K015801
23 03 30		3/138	10, 20, 30, 40, 60, 80, 100, 120, 150 mg/l MoO <sub>4</sub>	517631BT	Molybdate Tablets	13.5 mm cells DB 424	Industrial water systems	412920
23 36 00	NICKEL (Comparator)	3/36	1, 2, 3, 4, 5, 6, 7, 8, 10 mg		Dimethyl glyoxime	13.5 mm DB 424	Effluents	
23 01 70	NITRATE (Comparator)	3/124	0, 1, 0.2, 0.3, 0.4, 0.5, 0.6, 0.7, 0.8, 1.0 mg/l N	502810, 465230, 512310, 366220	Zinc reduction to nitrite (Nitrate Test Powder)	13.5 mm cells DB 424	Aquaria & drinking water	56K016001
23 17 00		3/17 ‡	5, 10, 20, 30, 40, 50, 60, 70, 80, 100 µg N		Pheno1.24 disulphonic acid	13.5 mm cells DB 424		
23 32 00		3/32 ‡	1, 2, 3, 4, 5, 6, 7, 8, 9 mg/l N		Brucine	13.5 mm cells DB 424		
23 56 00		3/17 ‡	10, 20, 40, 60, 80, 100, 120, 160, 200 µg N		Pheno1.24 disulphonic acid	13.5 mm cells DB 424		
23 03 60		3/142	10, 20, 30, 40, 50, 60, 70, 80, 100 mg/l N	517641	Nitrate No 1/No 2 tablets	13.5 mm cells DB 424		56K016101

‡ Laboratory method; not suitable as a test kit

Table of Lovibond® Water Test Discs

ORDER CODE	TEST (Instrument)	DISC CODE	DISC READINGS / RANGE COVERED	REAGENT CODE	CHEMICAL METHOD BASED ON	ACCESSORIES REQUIRED	KIT PART NUMBER
23 32 00	NITRATE (Comparator) <i>continued</i>	3/32 #	1, 2, 3, 4, 5, 6, 7, 8, 9 mg/l N	Brucine	13.5 mm cells DB 424		
23 56 00		3/56	10, 20, 40, 60, 80, 100, 120, 160, 200 µg N	Phenol 2:4 disulphonic acid	13.5 mm cells DB 424		
28 35 70	NITRATE (Nessleriser 2150)	NHP #	2.5, 5, 7.5, 10, 12.5, 15, 20, 25, 30 µg N	Phenol 2:4 disulphonic acid	Nessler cylinders AF 306/P		
28 35 60		NH #	2, 4, 6, 8, 10, 12, 15, 18, 25 µg N	2:4-xylene-t-oil	Nessler cylinders AF 306/P		56K016201
23 00 30	NITRITE (Comparator)	3/103	0.05, 0.1, 0.15, 0.2, 0.25, 0.3, 0.35, 0.4, 0.5 mg/l N	512310	Nitrite Low Range Tablets	13.5 mm cells DB 424	
23 83 00		3/83	1, 2, 3, 5, 7, 9, 11, 13, 15 µg N	Cleve's Acid	13.5 mm cells DB 424		
23 93 10		3/93A	0.02, 0.03, 0.04, 0.05, 0.06, 0.07, 0.08, 0.09, 0.1%	Cleve's Acid	25 mm cells W680/OG/25		
23 93 20		3/93B	0.10, 0.11, 0.12, 0.14, 0.15, 0.16, 0.18, 0.20%	Cleve's Acid	25 mm cells W680/OG/25		
28 39 60	NITRITE (Nessleriser 2150)	NJP	0.002, 0.004 0.006, 0.01, 0.015, 0.02, 0.03, 0.04, 0.05 mg/l N	512310, 502371	Nitrite LR Tablets	Nessler cylinders AF 306/P	
28 35 80		NJU	0.05, 0.1, 0.2, 0.3, 0.4, 0.5, 0.6, 0.8, 1.0 µg N	Cleve's Acid	Nessler cylinders AF 306/P		
	NITROGEN		(See Ammonia, Nitrate, Nitrite)				
23 03 00	OXYGEN, DISSOLVED (Comparator)	3/3	4, 5, 6, 7, 8, 9, 10, 11, 12 mg/l	461150, 461160,	Alsterberg's Method	13.5 mm cells DB 424	
23 06 50		3/165	2, 3, 4, 5, 6, 7, 8, 10, 12 mg/l	461170	" "	13.5 mm cells DB 424	
28 36 80	OXYGEN, DISSOLVED (Nessleriser 2150)	NOE	0, 0.005, 0.01, 0.015, 0.03, 0.055, 0.08, 0.1, 0.12 ml/l	"	Indigo carmine	Special glass cylinders AF 315	
28 35 90		NKA	0.05, 0.1, 0.2, 0.3, 0.4, 0.5, 0.6, 0.8, 1.0 ml/l	461150, 461160,	Alsterberg's Method	Nessler cylinders AF 306/P	
28 36 00		NKB	0.4, 0.5, 0.6, 0.7, 0.8, 1.0, 1.2, 1.4, 1.6 mg/l	461170	" "	Alsterberg's Method	
28 39 00		NYA #	0.001, 0.003, 0.005, 0.007, 0.009, 0.012, 0.015, 0.018, 0.02 ml/l	"	Modification of Alsterberg's Method	Nessler cylinders AF 306/P	
28 39 10		NYB #	0.025, 0.03, 0.035, 0.04, 0.045, 0.05, 0.06, 0.08, 0.1 ml/l	461150, 461160	Modification of Alsterberg's Method	Nessler cylinders AF 306/P	
28 38 00		NOWA #	0.002, 0.003, 0.005, 0.006, 0.008, 0.01, 0.011, 0.013, 0.014 ml/l	"	Acid o-Tolidine *	Nessler cylinders AF 306/P	
28 38 10		NOWB #	0.016, 0.024, 0.032, 0.04, 0.047, 0.053, 0.063, 0.071, 0.079 ml/l	"	Acid o-Tolidine *	Nessler cylinders AF 306/P	
23 67 00	OZONE (Comparator)	3/67	0, 1, 0.2, 0.3, 0.4, 0.5, 0.6, 0.7, 0.8, 1.0 mg/l	511220BT, 512170BT	DPD Tablets	13.5 mm cells DB 424	
23 67 10		3/67A	0.01, 0.02, 0.03, 0.04, 0.05, 0.06, 0.07, 0.08, 0.10 mg/l	"	DPD Tablets	40 mm cells DB 428	
23 67 70		3/67S	0.05, 0.1, 0.15, 0.2, 0.25, 0.3, 0.35, 0.4, 0.45 mg/l	"	DPD Tablets	13.5 mm cells, DB 424	
23 04 40		3/148	0, 0.05, 0.10, 0.15, 0.20, 0.25, 0.30, 0.40, 0.50 mg/l	513170	Ozone Tablets	40 mm cells DB 428	
28 37 60	OZONE (Nessleriser 2150)	NOR	0.01, 0.02, 0.04, 0.06, 0.1, 0.15, 0.2, 0.25, 0.3 mg/l	511261, 512170BT	DPD Tablets	Nessler cylinders AF 306/P	
28 37 70		NOS	0.2, 0.4, 0.6, 0.8, 1.0, 1.5, 2.0, 2.5 mg/l	Potassium Iodide	Nessler cylinders AF 306/P		
23 04 30	PERMANGANATE VALUE (Comparator)	3/3A	0, 5, 10, 15, 20, 30, 40, 50, 60 mg/l	Acid permanganate	13.5 mm cells DB 424	Approx. measure of oxidisable matter (organic & inorganic) in effluents & river water	

\* The use of o-Tolidine is controlled in the UK by the Carcinogenic Substances Regulations 1967    † Laboratory method; not suitable as a test kit

Table of Lovibond® Water Test Discs

ORDER CODE	TEST (Instrument)	DISC CODE	DISC READINGS / RANGE COVERED	REAGENT CODE	CHEMICAL METHOD BASED ON	ACCESSORIES REQUIRED	APPLICATIONS	KIT PART NUMBER
22 12 60	pH VALUE (Comparator) Narrow range	2/1Y	0.2, 0.4, 0.6, 0.8, 1.0, 1.2, 1.4, 1.6, 1.8	511600	Cresol Red	13.5 mm cells DB 424	Almost any aqueous solution. Nessler method more suitable for unbuffered water	
22 12 50		2/1W	1.0, 1.2, 1.4, 1.6, 1.8, 2.0, 2.2, 2.4, 2.6	511710	m-Cresol Purple	13.5 mm cells DB 424		
22 10 10		2/1A	1.2, 1.4, 1.6, 1.8, 2.0, 2.2, 2.4, 2.6, 2.8	511650	Thymol Blue	13.5 mm cells DB 424	"	"
22 10 30		2/1B	2.8, 3.0, 3.2, 3.4, 3.6, 3.8, 4.0, 4.2, 4.4	511620	Bromophenol Blue	13.5 mm cells DB 424	"	"
22 13 30		2/1ZG	2.8, 3.0, 3.2, 3.4, 3.6, 3.8, 4.0, 4.2, 4.4		Methyl Orange	13.5 mm cells DB 424	"	"
22 12 40		2/1V	3.0, 3.2, 3.4, 3.6, 3.8, 4.0, 4.2, 4.4, 4.6		"BDH 3046"	13.5 mm cells DB 424	"	"
22 10 50		2/1C	3.6, 3.8, 4.0, 4.2, 4.4, 4.6, 4.8, 5.0, 5.2	511760	Brom cresol Green	13.5 mm cells DB 424	"	"
22 10 60		2/1CC	4.0, 4.5, 5.0, 5.5, 6.0, 6.5, 7.0, 7.5, 8.0		"BDH 4080"	13.5 mm cells DB 424	"	"
22 10 70		2/1D	4.4, 4.6, 4.8, 5.0, 5.2, 5.4, 5.6, 5.8, 6.0		"BDH 4460"	13.5 mm cells DB 424	"	"
22 10 80		2/1E	4.4, 4.6, 4.8, 5.0, 5.2, 5.4, 5.6, 5.8, 6.0	451631	Methyl Red	13.5 mm cells DB 424	"	"
22 10 90		2/1F	4.8, 5.0, 5.2, 5.4, 5.6, 5.8, 6.0, 6.2, 6.4		Chlorophenol Red	13.5 mm cells DB 424	"	"
22 11 00		2/1G	5.2, 5.4, 5.6, 5.8, 6.0, 6.2, 6.4, 6.6, 6.8	511730	Brom cresol Purple	13.5 mm cells DB 424	"	"
22 11 10		2/1H	6.0, 6.2, 6.4, 6.6, 6.8, 7.0, 7.2, 7.4, 7.6	511640BT	Bromo thymol Blue	13.5 mm cells DB 424	"	"
22 11 30		2/1J	6.8, 7.0, 7.2, 7.4, 7.6, 7.8, 8.0, 8.2, 8.4	511750BT	Phenol Red	13.5 mm cells DB 424	"	"
22 11 40		2/1K	7.2, 7.4, 7.6, 7.8, 8.0, 8.2, 8.4, 8.6, 8.8	511600	Cresol Red	13.5 mm cells DB 424	"	"
22 12 70		2/1Z	7.6, 7.8, 8.0, 8.2, 8.4, 8.6, 8.8, 9.0, 9.2	511710	m-Cresol Purple	13.5 mm cells DB 424	"	"
22 11 90		2/1L	8.0, 8.2, 8.4, 8.6, 8.8, 9.0, 9.2, 9.4, 9.6	511650	Thymol Blue	13.5 mm cells DB 424	"	"
22 12 30		2/1U	8.6, 8.8, 9.0, 9.2, 9.4, 9.6, 9.8, 10.0		"BDH 8610"	13.5 mm cells DB 424	"	"
22 13 20		2/1ZF	8.6, 8.8, 9.0, 9.2, 9.4, 9.6, 9.8, 10.0, 10.2		Phenolphthalein	13.5 mm cells DB 424	"	"
22 12 00		2/1M	9.0, 9.5, 10.0, 10.5, 11.0		"BDH 9011"	13.5 mm cells DB 424	"	"
22 12 20	pH VALUE (Comparator) Broad range	2/1P	4.0, 5.0, 6.0, 7.0, 8.0, 9.0, 9.4, 10.0, 11.0	451770	Universal	13.5 mm cells DB 424	"	"
22 13 10		2/1ZE	1, 3, 5, 6, 7, 8, 9, 11, 13		"BDH Full Range"	13.5 mm cells DB 424	"	"
28 11 10	pH VALUE (Nessleriser 2150)	NLM	1.2, 1.4, 1.6, 1.8, 2.0, 2.2, 2.4, 2.6, 2.8	511650	Thymol Blue	Nessler cylinders AF 306/P	Almost any aqueous solution. Nessler method more suitable for unbuffered water	
28 11 20		NLN	2.8, 3.0, 3.2, 3.4, 3.6, 3.8, 4.0, 4.2, 4.4	511620	Bromophenol Blue	Nessler cylinders AF 306/P		
28 11 50		NLR	3.0, 3.2, 3.4, 3.6, 3.8, 4.0, 4.2, 4.4, 4.6		"BDH 3046"	Nessler cylinders AF 306/P	"	"
28 10 10		NLA	3.6, 3.8, 4.0, 4.2, 4.4, 4.6, 4.8, 5.0, 5.2	511760	Brom cresol Green	Nessler cylinders AF 306/P	"	"
28 11 70		NLT	4.0, 4.5, 5.0, 5.5, 6.0, 6.5, 7.0, 7.5, 8.0		"BDH 4080"	Nessler cylinders AF 306/P	"	"
28 11 30		NLO	4.4, 4.6, 4.8, 5.0, 5.2, 5.4, 5.6, 5.8, 6.0		"BDH 4460"	Nessler cylinders AF 306/P	"	"
28 11 00		NLL	4.4, 4.6, 4.8, 5.0, 5.2, 5.4, 5.6, 5.8, 6.0	451631	Methyl Red	Nessler cylinders AF 306/P	"	"
28 10 20		NLB	5.2, 5.4, 5.6, 5.8, 6.0, 6.2, 6.4, 6.6, 6.8	511730	Brom cresol Purple	Nessler cylinders AF 306/P	"	"
28 10 30		NLC	6.0, 6.2, 6.4, 6.6, 6.8, 7.0, 7.2, 7.4, 7.6	511640BT	Bromo thymol Blue	Nessler cylinders AF 306/P	"	"
28 10 40		NLD	6.8, 7.0, 7.2, 7.4, 7.6, 7.8, 8.0, 8.2, 8.4	511750BT	Phenol Red	Nessler cylinders AF 306/P	"	"

† Laboratory method; not suitable as a test kit

Table of Lovibond® Water Test Discs

ORDER CODE	TEST (Instrument)	DISC CODE	DISC READINGS / RANGE COVERED	REAGENT CODE	ACCESSORIES REQUIRED	APPLICATIONS	KIT PART NUMBER
28 10 50	pH VALUE (Nessleriser 2150) Continued	NLE	7.2, 7.4, 7.6, 7.8, 8.0, 8.2, 8.4, 8.6, 8.8	511600	Cresol Red m-Cresol Purple Thymol Blue	Nessler cylinders AF 306/P Nessler cylinders AF 306/P	Almost any aqueous solution. Nessler method more suitable for unbuffered water "
28 10 90		NLK	7.6, 7.8, 8.0, 8.2, 8.4, 8.6, 8.8, 9.0, 9.2	511710	"		
28 10 60		NLF	8.0, 8.2, 8.4, 8.6, 8.8, 9.0, 9.2, 9.4, 9.6	511650	"		
28 10 70		NLG	9.0, 9.5, 10.0, 10.5, 11.0	451770	"BDH 9011" Universal "BDH Full Range"		
28 10 80		NLH	4.0, 5.0, 6.0, 7.0, 8.0, 9.0, 9.4, 10.0, 11.0		"		
28 11 80		NLU	1, 3, 5, 6, 7, 8, 9, 11, 13		"		
23 43 00	PHENOLS, MONOHYDRIC (Comparator)	3/43	0, 0.5, 1, 1.5, 2.0, 2.5, 3, 3.5, 4 µg		4 amino-antipyrine	13.5 mm cells DB 424 For phenol, ortho and meta substituted phenols	
28 38 30	PHENOLS, TOTAL TAR ACIDS (Nessleriser 2150)	NP	0.01, 0.02, 0.03, 0.04, 0.05, 0.06, 0.07, 0.08, 0.09 parts per 100, 000		Sulphanilic acid	Nessler cylinders AF 306/P	Road run-off
23 02 70	PHOSPHATE* (Comparator)	3/133	0, 0.25, 0.5, 1.0, 1.5, 2.0, 2.5, 3.0, 4.0 mg/l PO <sub>4</sub>	517652BT	Phosphate Low Range Tablets	13.5 mm cells DB 424	
23 03 10		3/136	0, 5, 10, 15, 20, 25, 30, 35, 40 mg/l PO <sub>4</sub>	511980	Phosphate High Range Tablets	13.5 mm cells DB 424	
23 07 00		3/7	20, 40, 60, 80, 100, 130, 160, 190, 220 µg P <sub>2</sub> O <sub>5</sub>		Ammonium molybdate & stannous chloride	13.5 mm cells DB 424	
23 04 00		3/4 ‡	5, 10, 20, 30, 40, 50, 60, 80, 100 µg P <sub>2</sub> O <sub>5</sub>		Ammonium molybdate & metal	13.5 mm cells DB 424	
23 12 00		3/12	0, 10, 20, 30, 40, 50, 60, 70, 80 mg/l PO <sub>4</sub>		Ammonium molybdate & hydroquinone	13.5 mm cells DB 424	
23 38 00		3/38	10, 20, 30, 40, 50, 60, 70, 80, 100 mg/l PO <sub>4</sub>		Ammonium molybdate/vanadate	13.5 mm cells DB 424	
23 51 00		3/51 ‡	2, 5, 10, 15, 20, 30, 40, 60, 80 mg/l PO <sub>4</sub>		Ammonium molybdate & ascorbic acid	13.5 mm cells DB 424	
23 60 00		3/60	10, 20, 30, 40, 50, 60, 80, 100 mg/l PO <sub>4</sub>	56R017490	Vanadomolybdate single reagent	13.5 mm cells DB 424	
23 70 00		3/70	0, 10, 20, 30, 40, 50, 60, 80, 100 mg/l PO <sub>4</sub>	511980	Phosphate High Range Tablets	13.5 mm cells DB 424	
28 36 10	PHOSPHATE* (Nessleriser 2150)	NMB ‡	2, 4, 6, 8, 10, 12, 14, 17, 20 µg P <sub>2</sub> O <sub>5</sub>		Ammonium molybdate & stannous chloride	Nessler cylinders AF 306/P	
28 36 20		NMC ‡	5, 10, 15, 20, 25, 30, 40, 50, 60 µg P <sub>2</sub> O <sub>5</sub>		Ammonium molybdate & metal	Nessler cylinders AF 306/P	
28 37 50		NOP	10, 20, 30, 40, 50, 60, 70, 80, 100 µg PO <sub>4</sub>		Phosphate Nessleriser Tablets	Nessler cylinders AF 306/P	
28 38 20		NOX	1, 2, 3, 4, 5, 6, 7, 8, 10 mg/l PO <sub>4</sub>		Phosphate Nessleriser Tablets	Nessler cylinders AF 306/P	
28 39 50		NMD ‡	10, 20, 30, 40, 50, 60, 70, 80, 100 µg PO <sub>4</sub>		Ammonium molybdate / ascorbic acid	Nessler cylinders AF 306/P	
	PHOSPHORUS		See Phosphate				
	PLATINUM-COBALT COLOUR		See Hazen Colour				
23 01 20	QUATERNARY AMMONIUM COMPOUNDS (Comparator)	3/118	0, 2, 4, 6, 8, 10, 12, 15, 20 mg/l active QAC	515390	QAC Low Range Tablets	40 mm cells W680/OG/40	Swimming pools, cooling towers
23 01 30		3/119	0, 20, 40, 60, 80, 100, 120, 150, 200 mg/l active QAC	515400	QAC High Range Tablets	13.5 mm cells, DB 424	Washing & rinse water

\* Without pretreatment all colorimetric methods respond only to orthophosphate    † Laboratory method; not suitable as a test kit

56K017701

Table of Lovibond® Water Test Discs

ORDER CODE	TEST (Instrument)	DISC CODE	DISC READINGS / RANGE COVERED	REAGENT CODE	CHEMICAL METHOD BASED ON	ACCESSORIES REQUIRED	APPLICATIONS	KIT PART NUMBER
23 03 40	SILICA (SiO <sub>2</sub> ) (Comparator)	3/139	0.4, 0.6, 1.0, 1.5, 2.0, 2.5, 3.0, 3.5, 4.0 mg/l	517672	Silica Tablets	13.5 mm cells DB 424	Natural & treated water	411980
23 04 20		3/147	1, 2, 3, 4, 5, 6, 7, 8, 10 mg/l	517672	Silica Tablets	13.5 mm cells DB 424	Boiler water	56K017901
23 02 50		3/140	0.1, 0.2, 0.3, 0.4, 0.5, 0.6, 0.7, 0.8, 1.0 mg/l	460241	1-Amino-2-naphtho-4-sulphonic acid	40 mm cells DB 428		56K018001
23 13 00		3/13 ‡	2.5, 5, 7.5, 10, 12.5, 15, 17.5, 20, 25 mg/l	460241	Ammonium molybdate	40 mm cells DB 428		
28 36 30	SILICA (SiO <sub>2</sub> ) (Nessleriser 2150)	NN ‡	1, 2, 4, 6, 8, 10, 12, 16, 20 mg/l	460241	Ammonium molybdate	Nessler cylinders AF 306/P	"Take-off boost" water in jet aircraft	
28 36 40		NN	2, 3 mg/l only	460241	Ammonium molybdate	Nessler cylinders AF 306/P		
28 38 80		Special ‡	0.2, 0.3, 0.4, 0.5, 0.6, 0.7, 0.8, 0.9, 1.0 mg/l	460241	1-Amino-2-naphtho-4-sulphonic acid	Nessler cylinders AF 306/P	Boiler water	
	SODIUM HYPOCHLORITE		See Chlorine, Disc Code 3/2 Hypo					
23 29 10	SUGAR (Comparator)	3/29A	0, 5, 10, 15, 30, 45, 60, 75, 100 mg/l		alpha-Naphthol	5 mm cells W680/O/G/5	Sugar in boiler water or drain water in sugar refineries	
23 02 10	SULPHIDE (Comparator)	3/128	0, 0.05, 0.10, 0.15, 0.20, 0.25, 0.30, 0.40, 0.50 mg/l S	502930, 502940	Sulphide Tablets	13.5 mm cells DB 424	Fresh water and lightly polluted effluents	
23 01 60	SULPHITE (Comparator)	3/123	5, 10, 15, 20, 25, 30, 35, 40, 50 mg/l Na <sub>2</sub> SO <sub>3</sub>		Potassium iodide/iodate	40 mm cells DB 428	Boiler water	
28 36 50	SULPHITE (Nessleriser 2150)	NOB	2, 5, 10, 15, 20, 25, 30, 40, 50 mg/l Na <sub>2</sub> SO <sub>3</sub>		Potassium iodide/iodate	Nessler cylinders AF 306/P	Boiler water	
23 39 90	SWIMMING POOLS (Comparator)	3/40CZ	0.5, 1.0, 1.5, 2.0, 4.0 mg/l Cl <sub>2</sub> ; 7.0, 7.4, 7.6, 8.0 pH	511050BT, 511080BT, 511750BT	DPD Tablets for Chlorine Phenol Red for pH	13.5 mm cells DB 424	Combined disc with restricted ranges	
23 40 50		3/40D	0.5, 1, 2, 3, 4, 6 mg/l Cl <sub>2</sub> ; 7.0, 7.5, 8.0 pH	" " "	DPD Tablets for Chlorine, Phenol Red for pH	13.5 mm cells DB 424	Combined disc with restricted ranges	
23 06 10	TANNIN (Comparator)	3/161	0, 2, 4, 6, 8, 10, 12, 16, 20 mg/l Tannic acid		Folin & Ciocalteu's Reagent	13.5 mm cells DB 424	Corrosion inhibitors in industrial water systems	
23 63 00	THIOCYANATE (Comparator)	3/63 ‡	5, 10, 15, 20, 30, 40, 50, 60, 70 mg/l (SCN ion)		Ferric Chloride	10 mm cells W680/O/G/10	Effluent from carbonising plants	
23 35 00	TIN (Comparator)	3/35 ‡	1, 2, 3, 4, 5, 6, 8, 10, 12 mg/l		Dithiol	13.5 mm cells DB 424		
23 20 00	VANADIUM (Comparator)	3/20	10, 20, 30, 40, 50, 60, 70, 80, 100 µg		8-Hydroxyquinoline	13.5 mm cells DB 424		
23 69 00	ZINC (Comparator)	3/69	0, 2.5, 5, 10, 15, 20, 30, 40, 50 µg		Brilliant Green	13.5 mm cells DB 424		
		3/151	0, 0.1, 0.2, 0.3, 0.4, 0.5, 0.6, 0.8, 1.0 mg/l	512620BT	Copper/Zinc LR Tablets	13.5 mm cells DB 424	Industrial water/waste water	56K018201
23 04 70		3/145	0.02, 0.06, 0.1, 0.15, 0.2, 0.25, 0.3, 0.35, 0.4 mg/l	512620BT	Copper/Zinc LR Tablets	40 mm cells DB 428		
23 03 90		3/102	0, 0.5, 1.0, 1.5, 2.0, 2.5, 3.0, 3.5, 4.0 mg/l	512340BT	Copper/Zinc HR Tablets	13.5 mm cells DB 424		
23 00 20								56K018301

‡ Laboratory method; not suitable as a test kit



**The Tintometer Ltd**  
Lovibond House  
Solar Way  
Solstice Park  
Amesbury  
SP4 7SZ

Tel: +44 (0)1980 664800  
Fax: +44 (0)1980 625412

[water.sales@tintometer.com](mailto:water.sales@tintometer.com)

Lovibond® and Tintometer® are Registered Trademarks of The Tintometer Ltd. All translations and transliterations of LOVIBOND® & TINTOMETER® are asserted as Trade Marks of The Tintometer Ltd.

Registered Office: Lovibond House, UK. Registered in England No. 45024.

Errors and Omissions Excepted - Content subject to alteration without notice.

Version 05 \_ 06/13

[www.lovibondwater.com](http://www.lovibondwater.com)