


## Instruction Manual

# HI 93752 Calcium & Magnesium High Range ISM

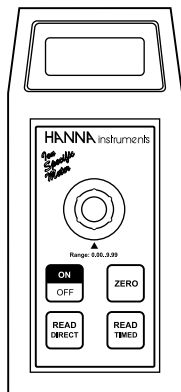

Dear Customer,

Thank you for choosing a Hanna product. This manual will provide you with the necessary information for the correct operation of the meter. Please read it carefully before using the meter. If you need additional technical information, do not hesitate to e-mail us at [tech@hannainst.com](mailto:tech@hannainst.com).

This instrument is in compliance with CE directives EN 50081-1 and EN 50082-1.

## PRELIMINARY EXAMINATION

Remove the instrument from the packing material and examine it carefully to make sure that no damage has occurred during shipment. If there is any damage, notify your Dealer.

Each Ion Specific Meter is supplied complete with


- 9V Battery
- Two Sample Cuvets and Caps
- One Transport Cap

Note: Conserve all packing material until the instrument has been observed to function correctly. Any defective item must be returned in its original packing.

## BATTERY REPLACEMENT

Battery replacement must only take place in a non-hazardous area using a 9V alkaline battery.

Simply slide off the battery cover on the back of the meter. Detach the battery from the terminals and attach a fresh 9V battery while paying attention to the correct polarity. Replace the battery and the cover.



## GENERAL DESCRIPTION

The HI 93752 meter measures the calcium content in the 0 to 400 mg/L (ppm) range and the magnesium content in the 0 to 150 mg/L (ppm) range in water and wastewater.


The meter uses an exclusive positive-locking system to ensure that the cuvet is in the same place every time it is placed into the measurement cell.

The reagents are in liquid form and are supplied in bottles. The amount of reagent is precisely dosed to ensure maximum repeatability.

Display codes aid the user in routine operations.

The meters have an auto-shut off feature that will turn the instrument off after 10 minutes of non-use.

## SPECIFICATIONS

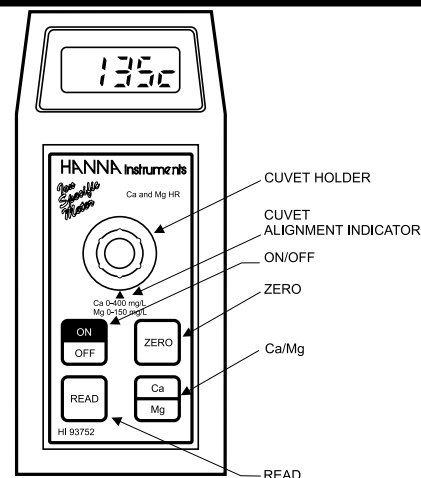

## SPECIFICATIONS

Range	0 to 400 mg/L (ppm) as Calcium 0 to 150 mg/L (ppm) as Magnesium
Resolution	1 mg/L
Accuracy	± 10 mg/L ± 5% of reading (Ca) ± 3 mg/L ± 3% of reading (Mg)
Typical EMC Deviation	± 1 mg/L
Light Source	Light Emitting Diode @ 470 nm
Method	To determine Calcium: Adaptation of the Oxalate method To determine Magnesium: Adaptation of the Calmagite method
Light Detector	Silicon Photocell
Environment	0 to 50°C (32 to 122°F); max 95% RH non-condensing
Battery Type/Life	1 x 9 volt/40 hours
Auto-Shut off	After 10' of non-use
Dimensions	180 x 83 x 46 mm (7.1 x 3.3 x 1.8")
Weight	290 g (10 oz.).

## REQUIRED REAGENTS

Code	Description	Quantity
-	Buffer Reagent	4 drops
HI 93752A-0 Ca	Calcium Buffer Reagent	7 mL
HI 93752B-0 Ca	Calcium Oxalate Reagent	1 mL
HI 93752A-0 Mg	Magnesium Buffer Reagent	1 mL
HI 93752B-0 Mg	Magnesium Indicator Reagent	9 mL

## DISPLAY CODE GUIDE

---	This indicates that the meter is in a ready state and zeroing can be performed.
5 IP	Sampling in Progress. This prompt appears each time the meter is performing a measurement.
-00-	This indicates that the meter is in a zeroed state and measurement can be performed.
2E00	A zero reading was not taken. Insert a sample before adding reagent and press ZERO.
0.00	Under range. A blinking "0.00" indicates that the sample absorbs less light than the zero reference. Check the procedure and make sure you use the same cuvet for reference (zero) and measurement.
330	Over range. A flashing value higher than the maximum concentration readable (see specifications) indicates that the sample absorbs too much light, meaning that the concentration is too high. Dilute the sample.
CAP	Light over range. The cuvet is not inserted correctly and an excess ambient light is reaching the detector. If the cover is properly installed, then contact your dealer or the nearest Hanna Customer Service Center.
L0	Light under range. The zero sample is too dark for proper zeroing. If this is not the case, contact your dealer or the nearest Hanna Customer Service Center.
V 250	The "V" indicates that the battery voltage is getting low and the battery needs to be replaced.
-88-	This indicates that the battery is dead and must be replaced. Note: once this indication is displayed, the meter will lockup. Change the battery to restart.

**HANNA**  
instruments  
[www.hannainst.com](http://www.hannainst.com)

**CE**  
This Instrument is in  
Compliance with the CE Directives

## WARRANTY

HI 93752 is warranted for two years against defects in workmanship and materials when used for its intended purpose and maintained according to instructions.

This warranty is limited to repair or replacement free of charge.

Damages due to accident, misuse, tampering or lack of prescribed maintenance are not covered.

If service is required, contact the dealer from whom you purchased the instrument. If under warranty, report the model number, date of purchase, serial number and the nature of the failure. If the repair is not covered by the warranty, you will be notified of the charges incurred. If the instrument is to be returned to Hanna Instruments, first obtain a Returned Goods Authorization Number from the Customer Service department and then send it with shipment costs prepaid. When shipping any instrument, make sure it is properly packaged for complete protection.

To validate your warranty, fill out and return the enclosed warranty card within 14 days from the date of purchase.




*All rights are reserved. Reproduction in whole or in part is prohibited without the written consent of the copyright owner, Hanna Instruments Inc., Woonsocket, Rhode Island, 02895, USA.*

Hanna Instruments reserves the right to modify the design, construction and appearance of its products without advance notice.


## OPERATIONAL GUIDE

### MEASUREMENT PROCEDURE TO DETERMINE CALCIUM


- Turn the meter on by pressing ON/OFF.
- When the LCD displays " - - - ", it is ready.
- Select Calcium by pressing Ca/Mg. A "c" will appear on the right corner of the display.
- Using the 5 mL syringe add exactly 3.00 mL of sample to the cuvet.





probable level of liquid taken up by syringe




- Add 4 drops of Buffer Reagent.




- Use the pipette to fill the cuvet up to the 10 mL mark with the HI 93752A-0 Ca reagent.
- Replace the cap and invert several times to mix.
- Place the cuvet into the holder and ensure that the notch on the cap is positioned securely into the groove.




- Press ZERO and "SIP" will appear on the display.





- Wait for a few seconds and the display will show "-0.0-". Now the meter is zeroed and ready for measurement.
- Remove the cuvet.



- Using the 1 mL syringe, add exactly 1 mL of the HI 93752B-0 Ca Oxalate reagent. Replace the cap and invert the cuvet 10 times to mix.



- Wait for 5 minutes, then invert again the cuvet 10 times and after that reinsert the cuvet into the instrument.



- Wait for 10 seconds, press READ and SIP will appear on the display.
- The instrument directly displays concentration in mg/L of Calcium on the Liquid Crystal Display.







Note: To ensure accurate results, perform the tests at room temperature, between 18°C and 28°C (65F to 83F).

Interferences:

	concentration	reading
Acidity (as CaCO <sub>3</sub> )	above 1000 mg/L	lower
Alkalinity (as CaCO <sub>3</sub> )	above 1000 mg/L	higher
Magnesium (Mg <sup>2+</sup> )	above 400 mg/L	higher

### MEASUREMENT PROCEDURE TO DETERMINE MAGNESIUM

- Select Magnesium by pressing Ca/Mg. An "m" will appear on the right corner of the display.
- Using one 1 mL syringe add exactly 1.00 mL of HI 93752A-0 Mg Buffer reagent to the cuvet and use the pipette to fill the cuvet up to the 10 mL mark with the HI 93752B-0 Mg Indicator reagent.
- Replace the cap and invert several times to mix.
- Place the cuvet into the holder and ensure that the notch on the cap is positioned securely into the groove.
- Press ZERO and "SIP" will appear on the display.
- Wait for a few seconds and the display will show "-0.0-". Now the meter is zeroed and ready for measurement.
- Remove the cuvet.
- Using the other 1 mL syringe, add to the cuvet exactly 0.5 mL of sample.




Note: Do not mix up the two syringes!


- Replace the cap and invert several times to mix. Wait for 15 seconds.



- Reinsert the cuvet into the instrument.



- Press READ and SIP will appear on the display.



- The instrument directly displays concentration in mg/L of Magnesium on the Liquid Crystal Display.

Interferences:

	concentration	reading
Acidity (as CaCO <sub>3</sub> )	above 1000 mg/L	lower
Alkalinity (as CaCO <sub>3</sub> )	above 1000 mg/L	higher
Calcium (Ca <sup>2+</sup> )	above 200 mg/L	higher
Iron	-	higher
Aluminum	-	higher
Copper	-	higher

### FOR BEST RESULTS BOTH FOR CALCIUM AND MAGNESIUM DETERMINATION:

Intensely colored samples will cause interference, therefore they should be adequately treated before performing the test. Suspended matter in large amounts should be removed by prior filtration.

### ACCESSORIES FOR CALCIUM AND MAGNESIUM

- 1 syringe (5 mL) with tip
- 3 syringes (1 mL) with tips
- 2 plastic pipettes

### TIPS FOR AN ACCURATE MEASUREMENT

The instruction listed below should be carefully followed during testing to ensure best accuracy.

- Do not touch the cuvet walls with hands.
- In order to maintain the same conditions during the zeroing and the measuring phases, it is necessary to close the cuvet to prevent any contamination.
- Do not let the test sample stand too long after reagent is added or accuracy will be affected.
- Whenever the cuvet is placed into the measurement cell, it must be completely free of fingerprints, oil or dirt. Wipe it thoroughly with HI 731318 or a lint-free cloth prior to insertion.
- It is important that the sample does not contain any debris. This

would corrupt the readings.

- It is possible to take multiple readings in a row, but it is recommended that a zero reading be taken for each sample and that the same cuvet is used for zeroing and measurement.
- It is important to discard the sample immediately after the reading is taken because the glass might become permanently stained.
- Shaking the cuvet can generate bubbles in the sample, causing higher readings. To obtain accurate measurements, remove such bubbles by swirling or by gently tapping the vial.
- All the reaction times reported in this manual are referred to 20°C (68°F). As a general rule of thumb, they should be doubled at 10°C (50°F) and halved at 30°C (86°F).

## ACCESSORIES

### REAGENT SETS

HI 93752-01 Reagents for 100 tests

### OTHER ACCESSORIES

- HI 710009 Blue rubber boot
- HI 710010 Orange rubber boot
- HI 721310 9V battery (10 pcs)
- HI 731318 Tissue for wiping cuvetts (4 pcs)
- HI 731321 Glass cuvetts (4 pcs)
- HI 731325 Caps for cuvetts (4 pcs)
- HI 740142 1 mL graduated syringe
- HI 740143 1 mL graduated syringes (6 pcs)
- HI 740144 Pipette tip (6 pcs)
- HI 740157 Plastic refilling pipette (20 pcs)
- HI 93703-50 Cuvets cleaning solution (230 mL)
- C115-00300 5 mL graduated syringe

## CE DECLARATION OF CONFORMITY

Recommendations for Users

Before using these products, make sure that they are entirely suitable for the environment in which they are used.

Operation of these instruments in residential area could cause unacceptable interferences to radio and TV equipments, requiring the operator to take all necessary steps to correct interferences.

Any variation introduced by the user to the supplied equipment may degrade the instruments' EMC performance.

To avoid damages or burns, do not perform any measurement in microwave ovens.

